

212052US-2



IN THE UNITED STATES PATENT & TRADEMARK OFFICE

IN RE APPLICATION OF:
Tetsuya KAWAGISHI, et al.

: GROUP ART UNIT: N/A

SERIAL NO: 09/912,632

FILED: July 26, 2001

FOR: ULTRASONIC DIAGNOSIS APPARATUS AND ULTRASOUND IMAGING
METHOD

LETTER TO THE OFFICIAL DRAFTSMAN

ASSISTANT COMMISSIONER FOR PATENTS
WASHINGTON, DC 20231

SIR:

In response to the Notice to File Missing Parts of Nonprovisional Application, attached hereto please find 10 sheets of Substitute Formal Drawings. It is requested that the enclosed 10 sheets of Substitute Formal Drawings be entered to replace the drawings previously filed in this application.

Respectfully submitted,

OBLON, SPIVAK, McCLELLAND,
MAIER & NEUSTADT, P.C.

A handwritten signature in black ink, appearing to read "Joseph A. Scafetta Jr." or a similar variation.

Marvin J. Spivak
Attorney of Record
Registration No: 24,913

Joseph A. Scafetta, Jr.
Registration No. 26,803



22850
(703) 413-3000
Fax: (703) 412-2220
MJS/dgh
H:\Drawings\212052 subformals\trtooffdrfman.wpd

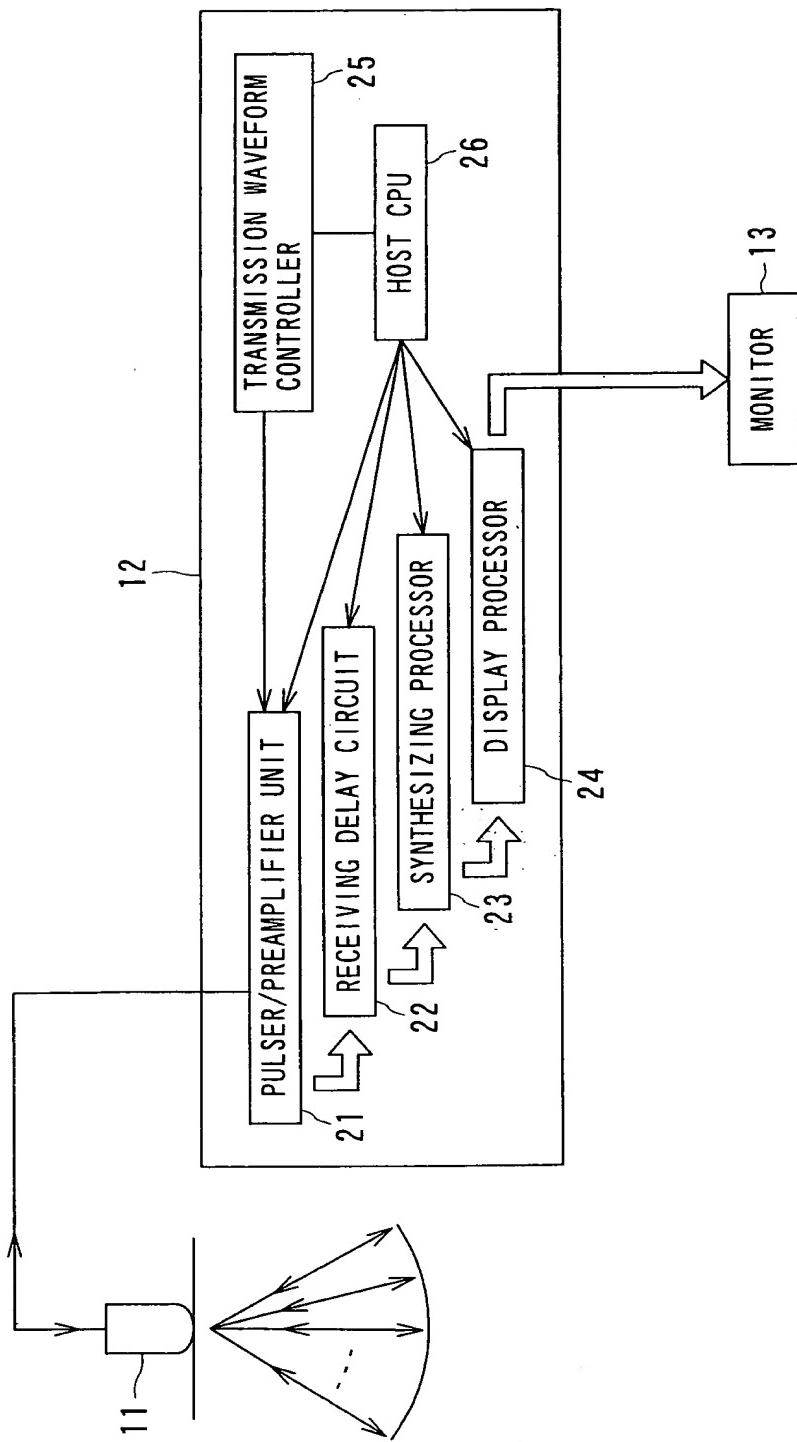


FIG. 1

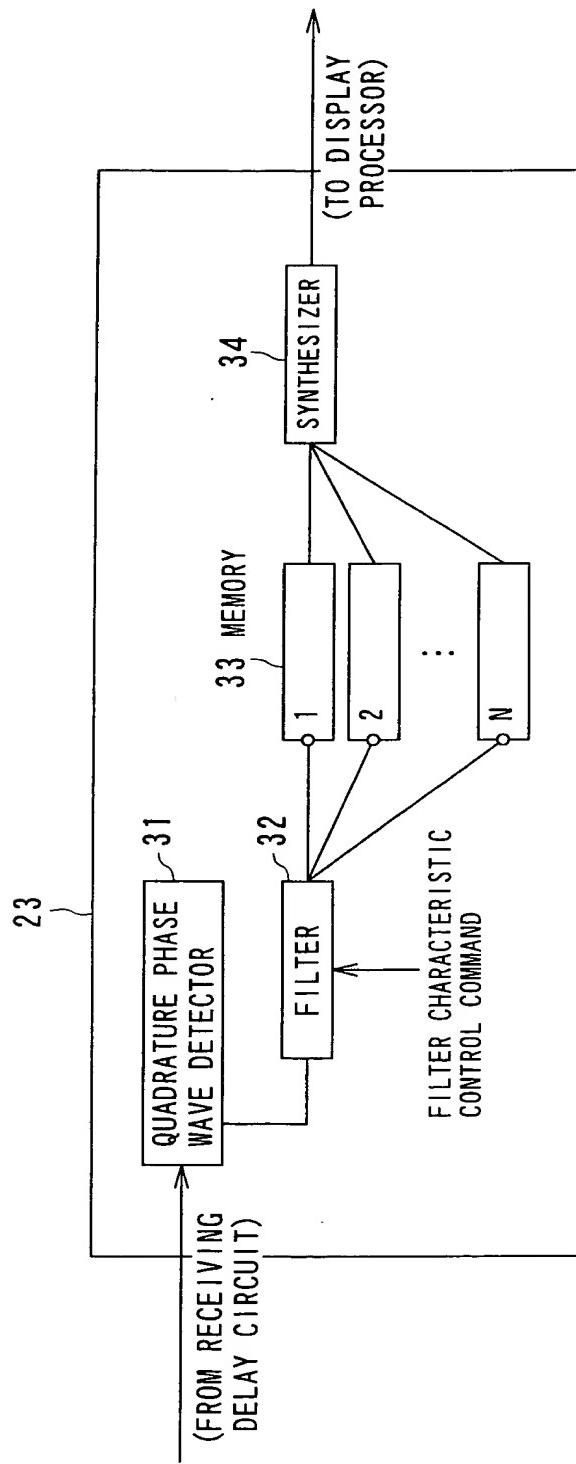


FIG. 2

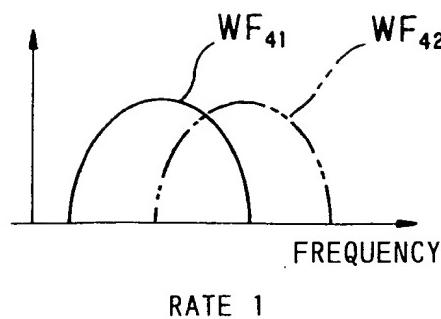


FIG. 3A

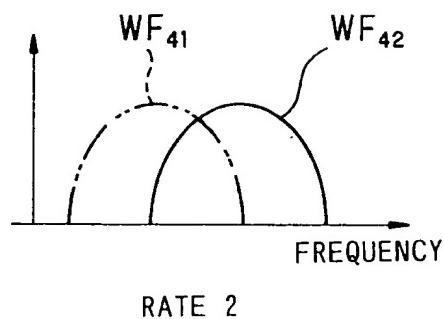


FIG. 3B

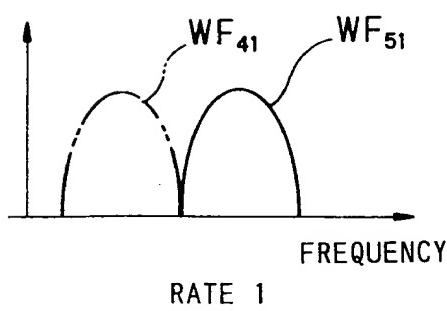


FIG. 4A

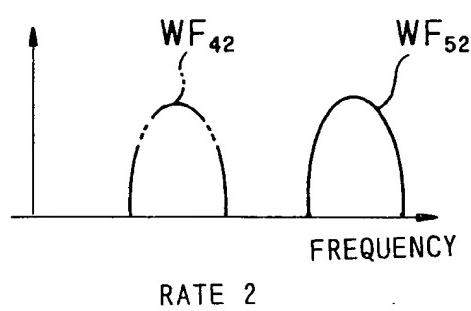


FIG. 4B

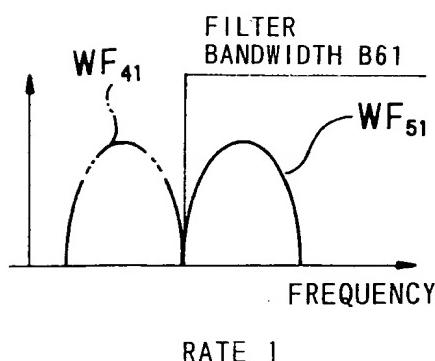


FIG. 5A


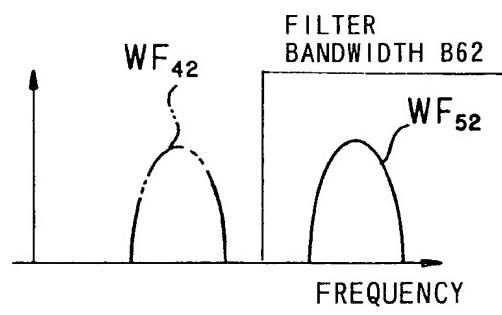



FIG. 5B

DRAFTED BY TETSUYA KAWAGISHI

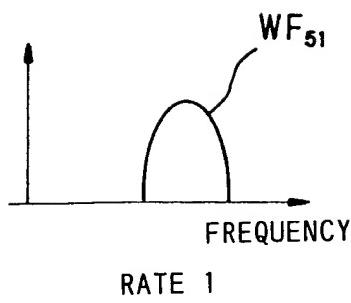

RATE 1

FIG. 6A

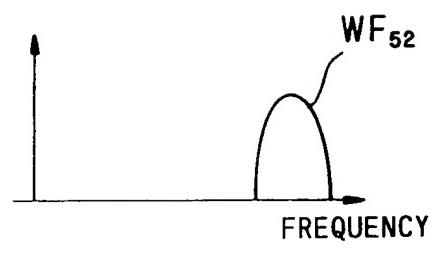

RATE 2

FIG. 6B

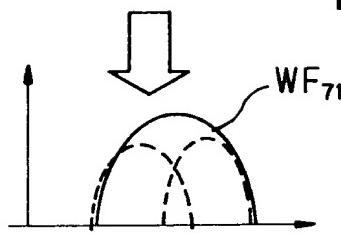


FIG. 6C

TOSATO 432922560

FIG. 7A

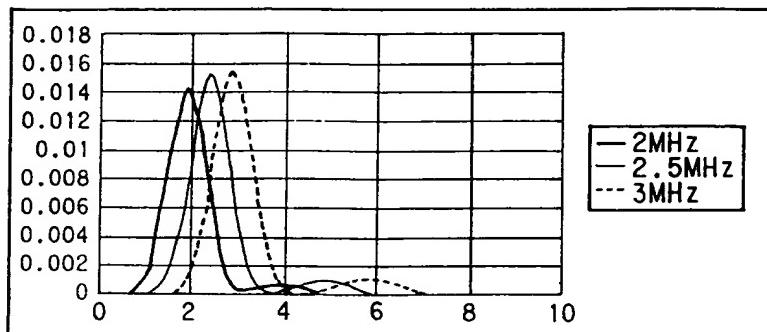


FIG. 7B

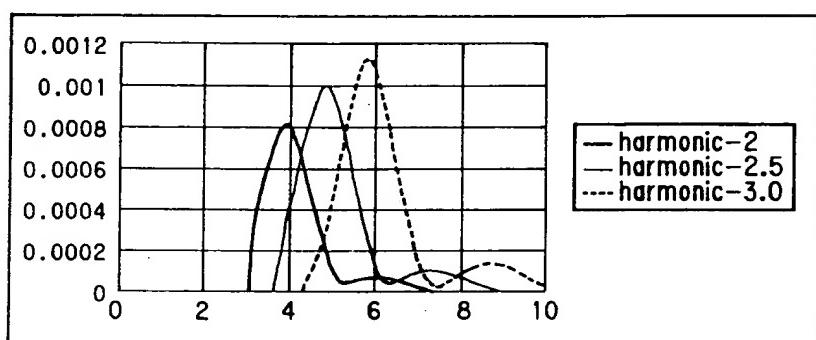


FIG. 7C

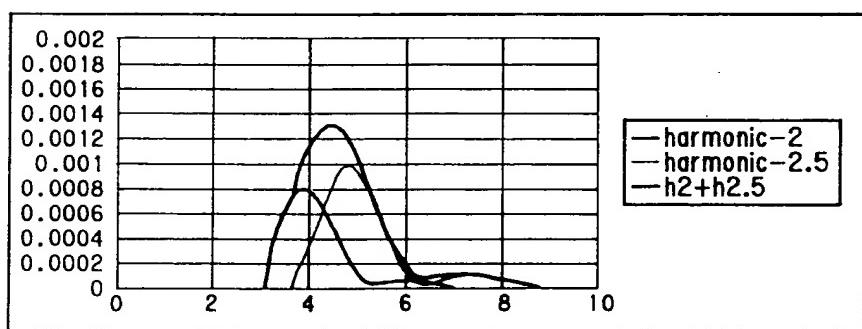


FIG. 7D

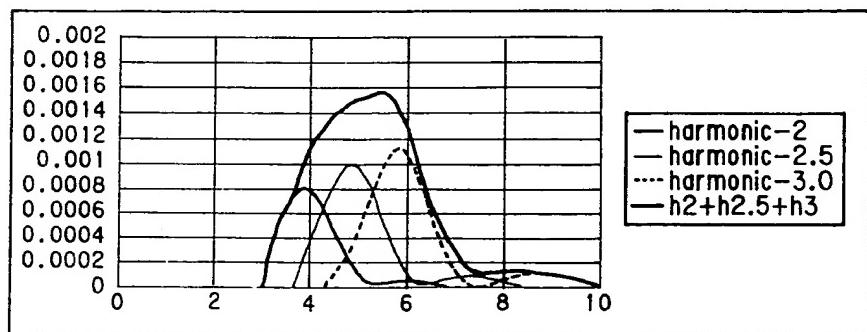


FIG 8A FIG 8B

OBLON, SPIVAK, et al.
SERIAL NO:09/912,632
INV: Tetsuya KAWAGISHI, ET AL.
DOCKET # 212052US-2
SHEET 6 OF 10

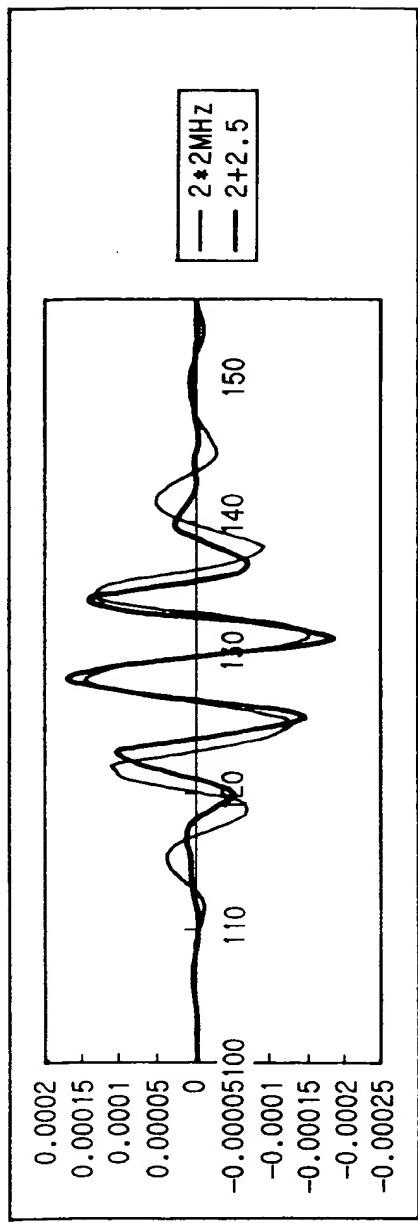


FIG. 8A

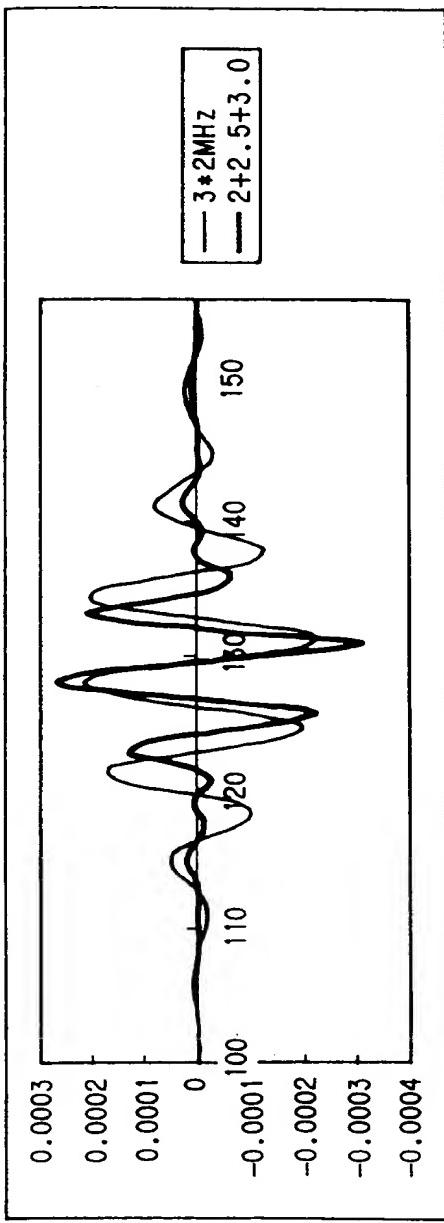


FIG. 8B

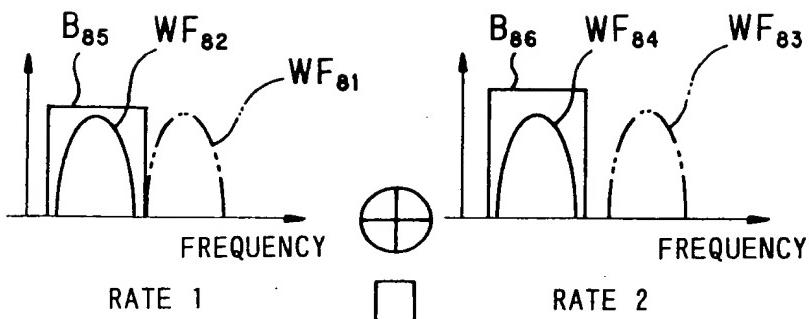


FIG. 9A

FIG. 9B

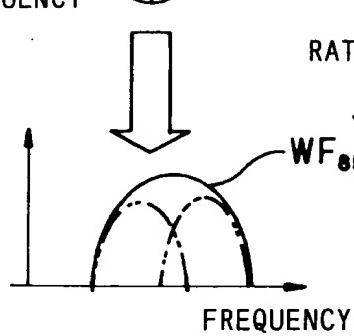


FIG. 9C

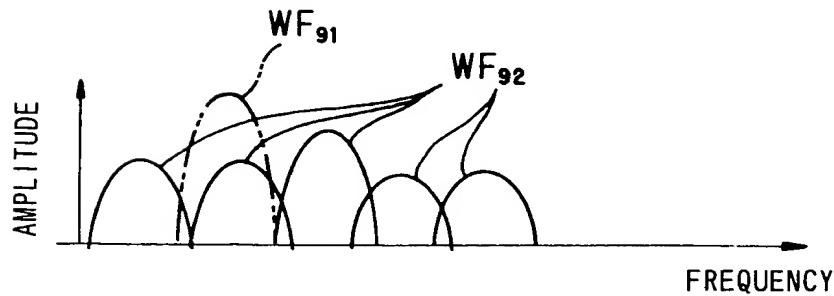


FIG. 10

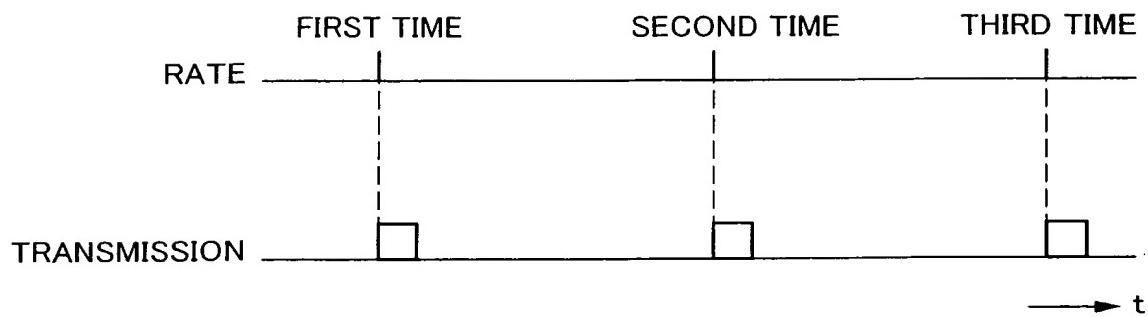


FIG. 11

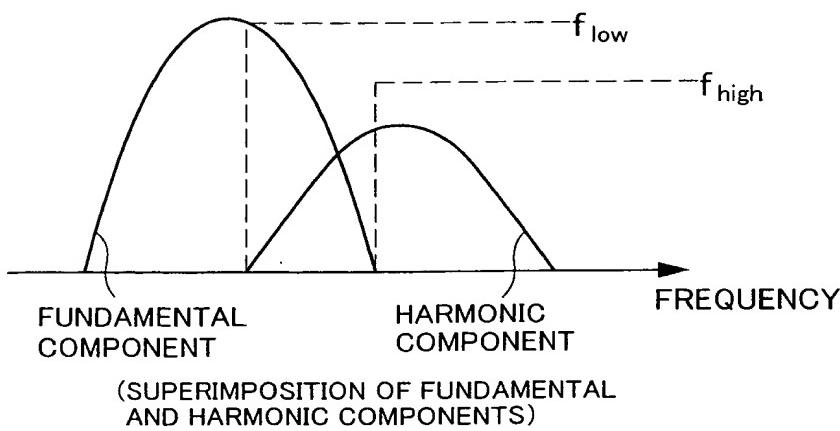


FIG. 12

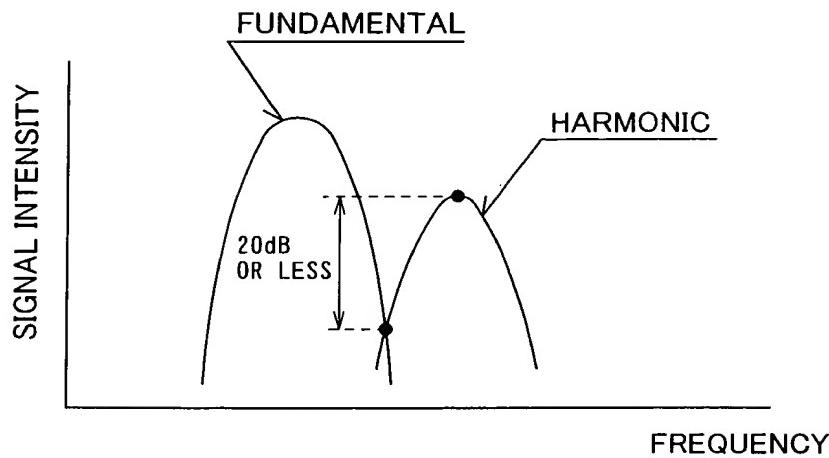


FIG. 13

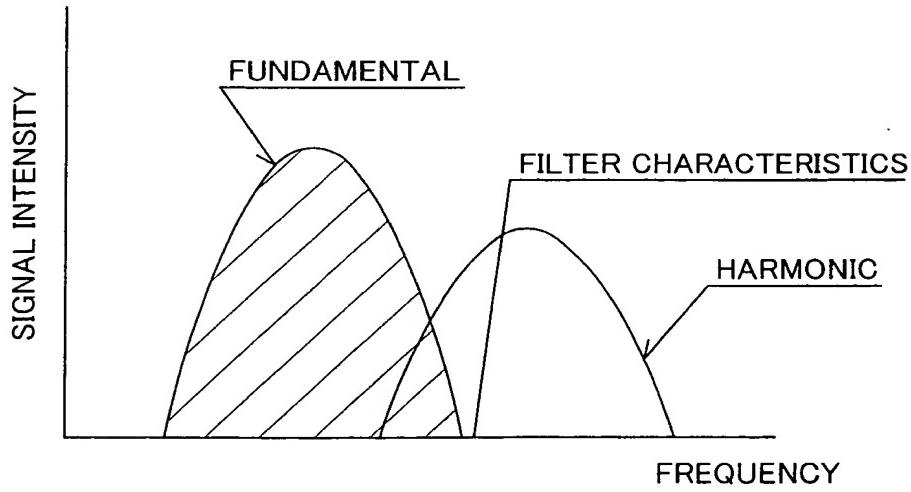


FIG. 14

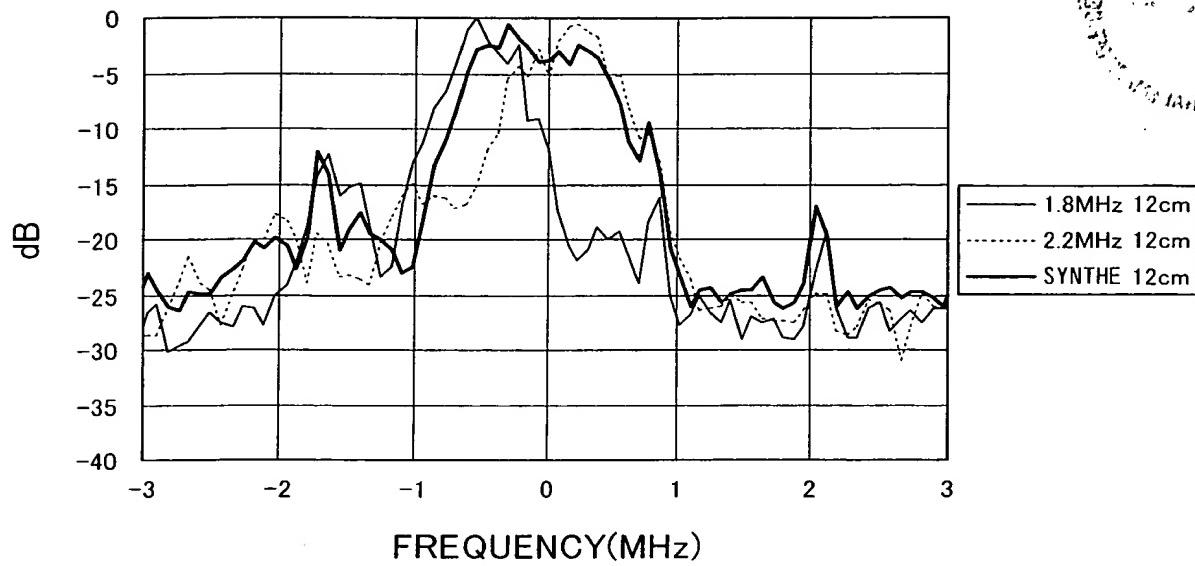


FIG. 15

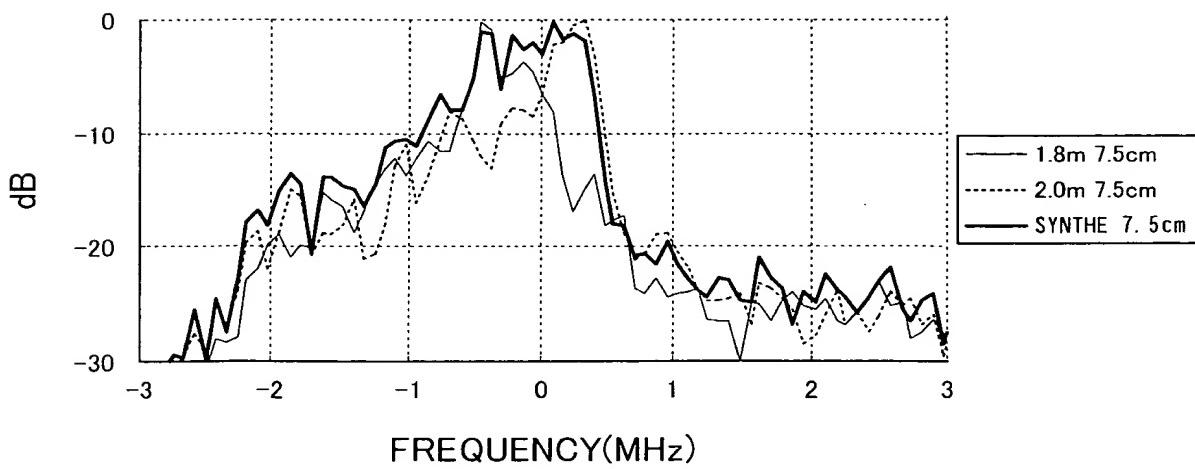


FIG. 16

FIG. 1

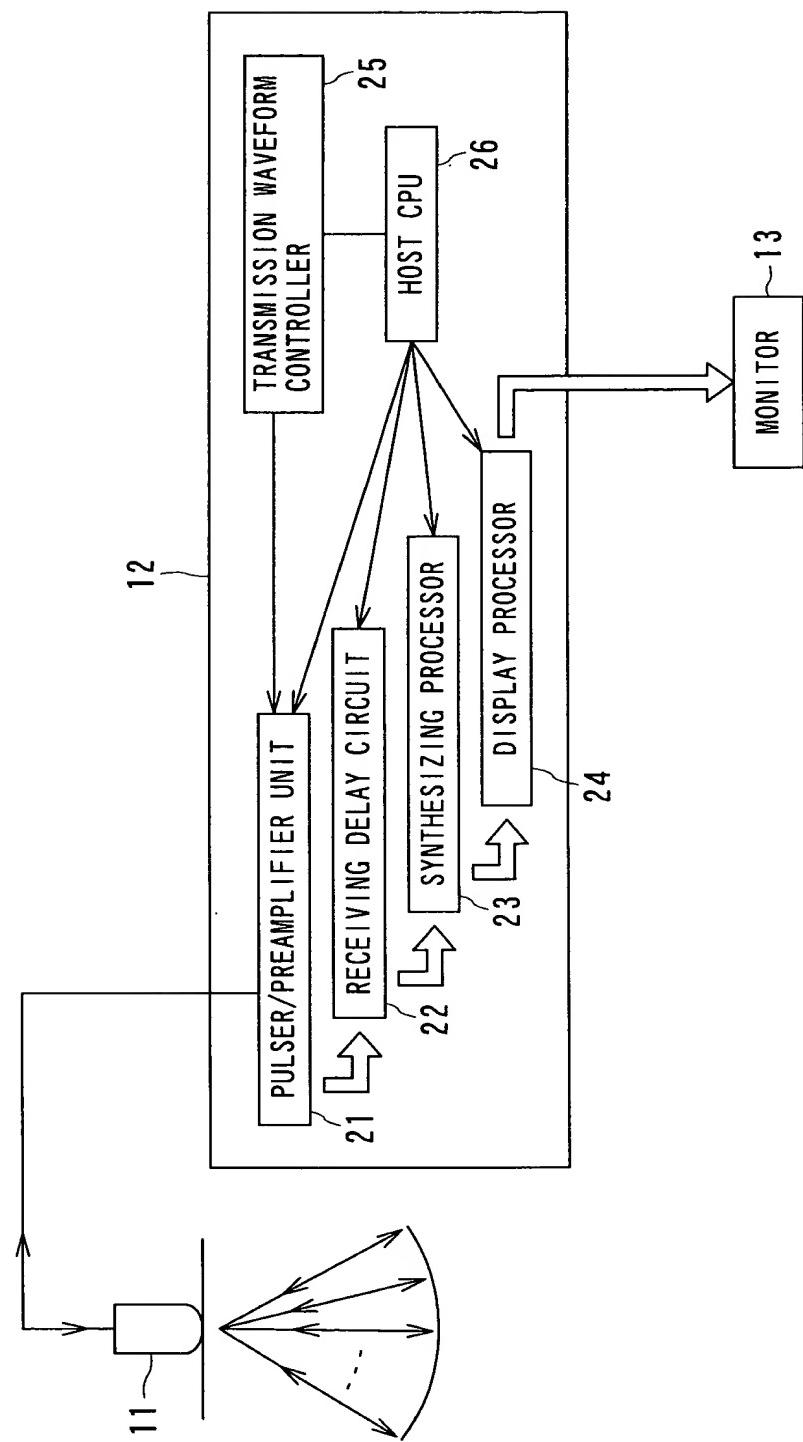
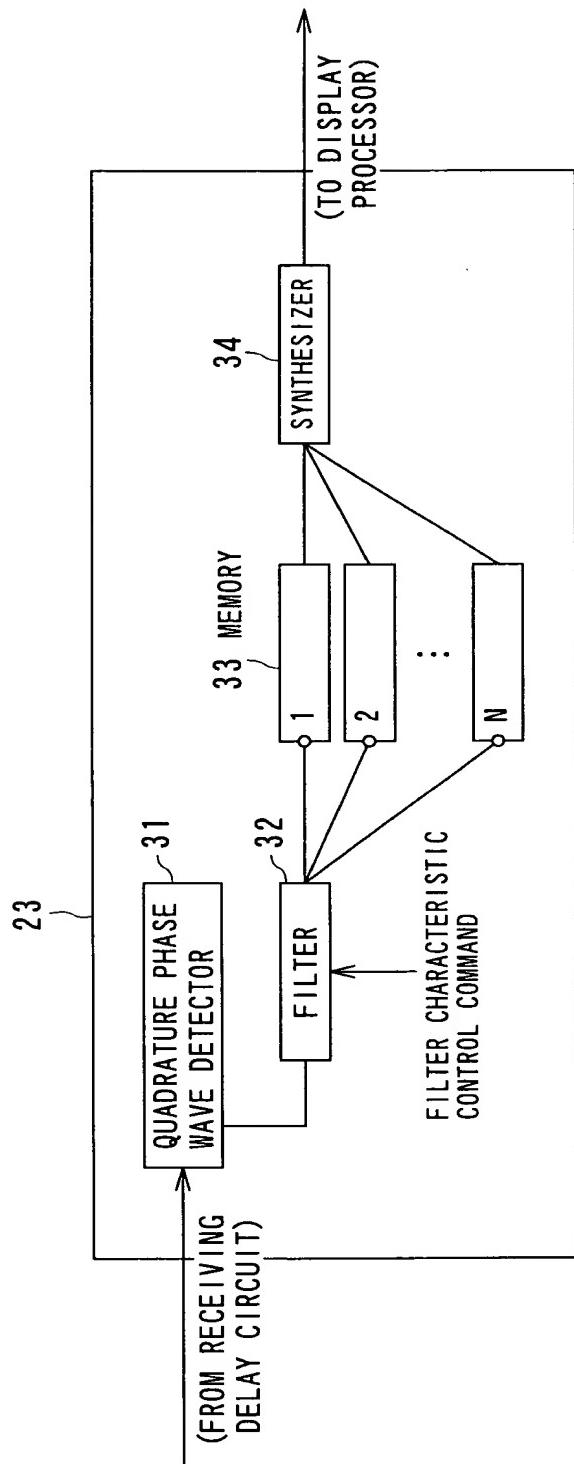


FIG. 2



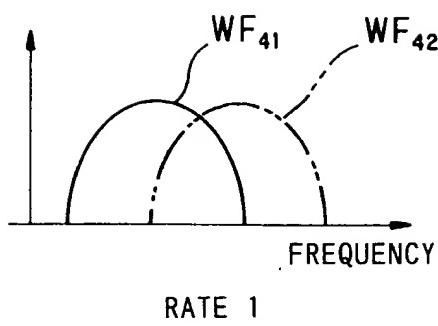


FIG. 3A

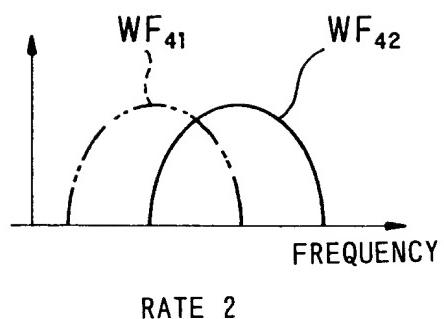


FIG. 3B

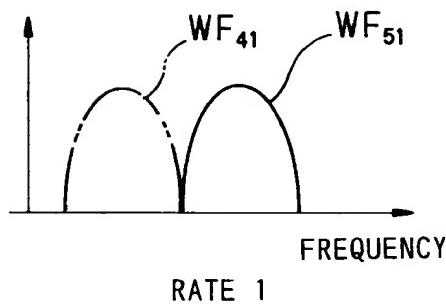


FIG. 4A

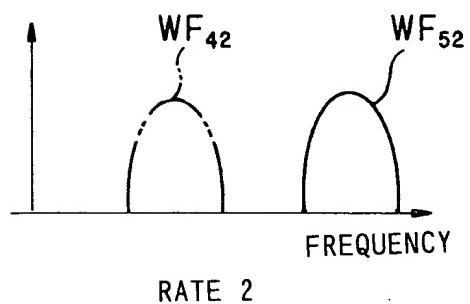


FIG. 4B

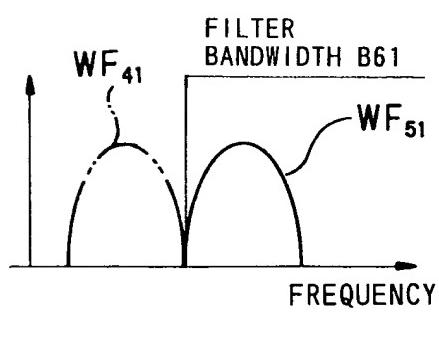


FIG. 5A

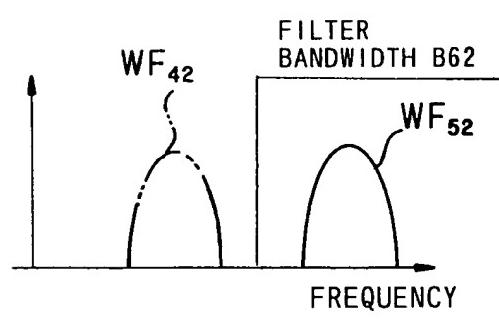


FIG. 5B


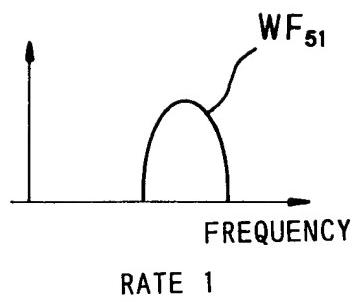


FIG. 6A

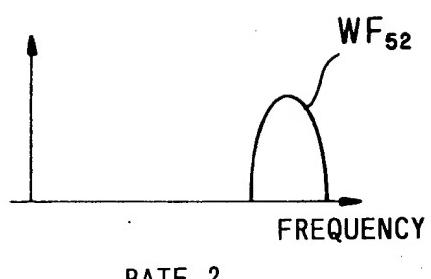

RATE 2

FIG. 6B

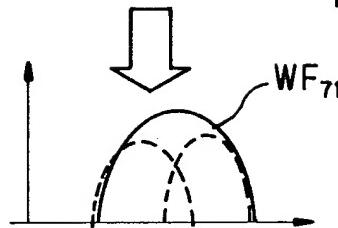


FIG. 6C

FIG. 7A

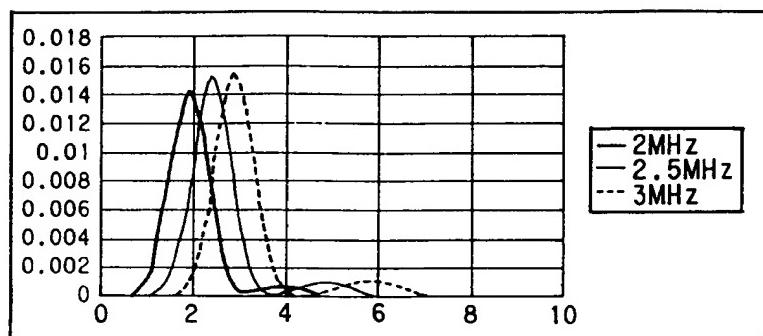


FIG. 7B

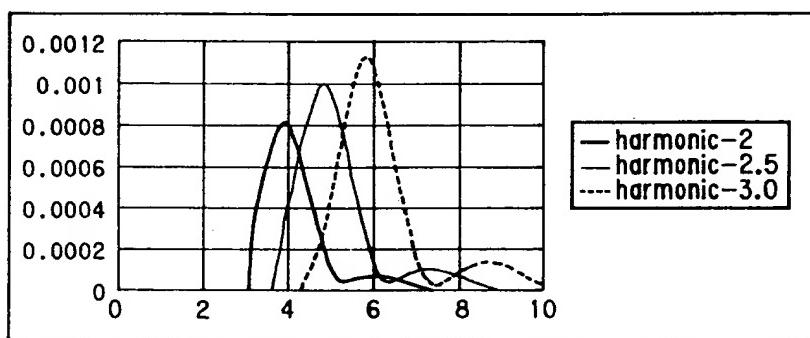


FIG. 7C

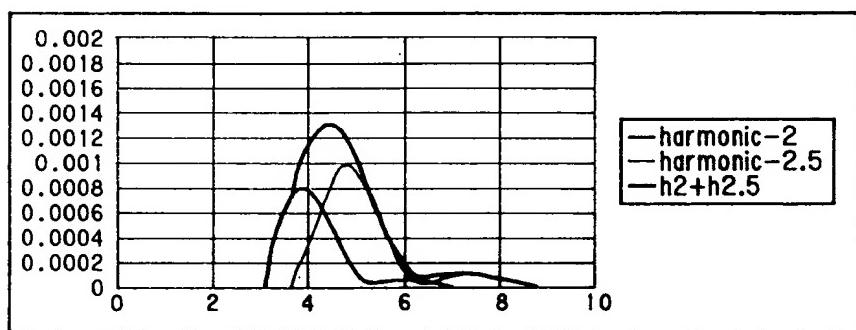


FIG. 7D

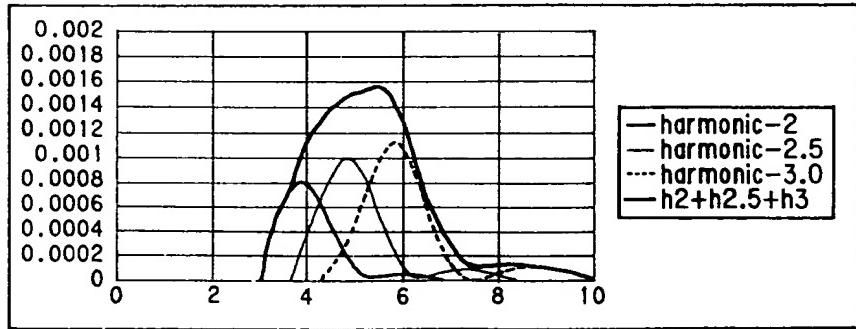


FIG. 8A




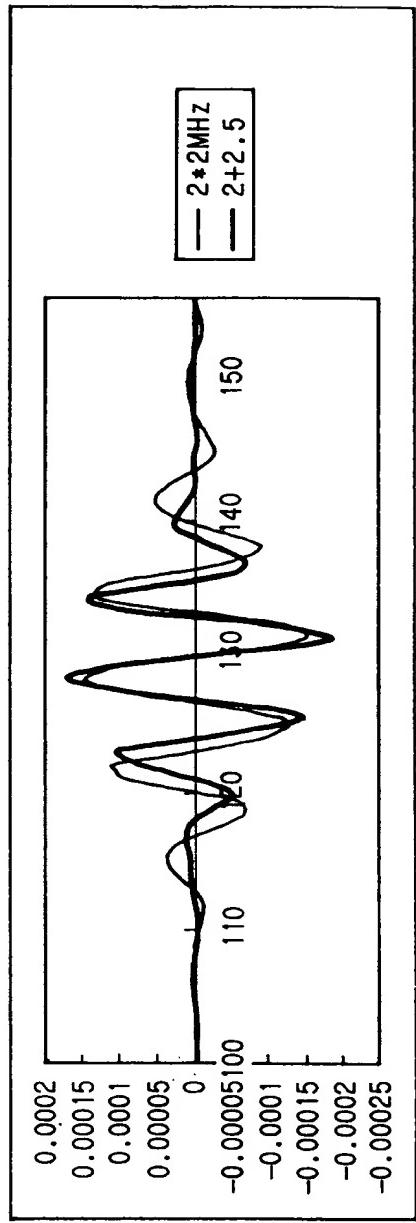


FIG. 8B


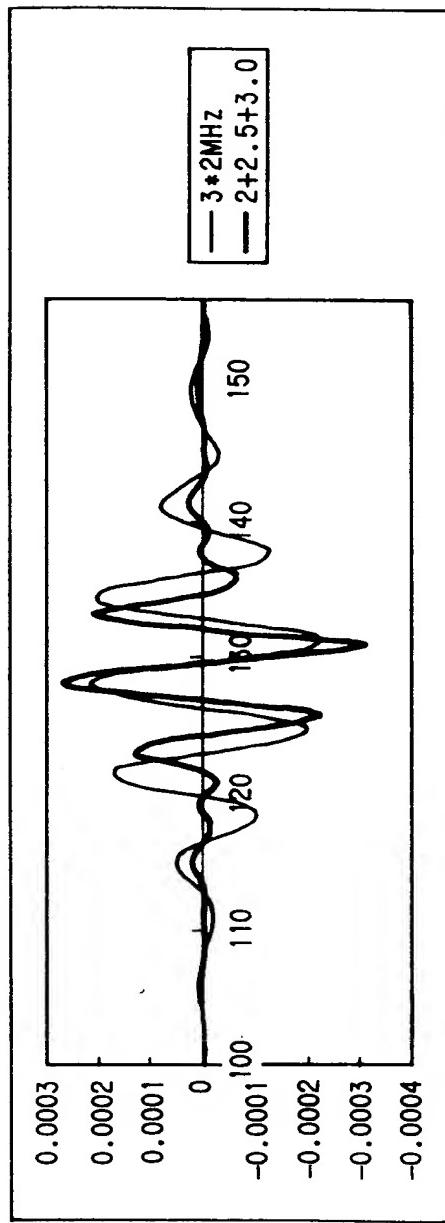


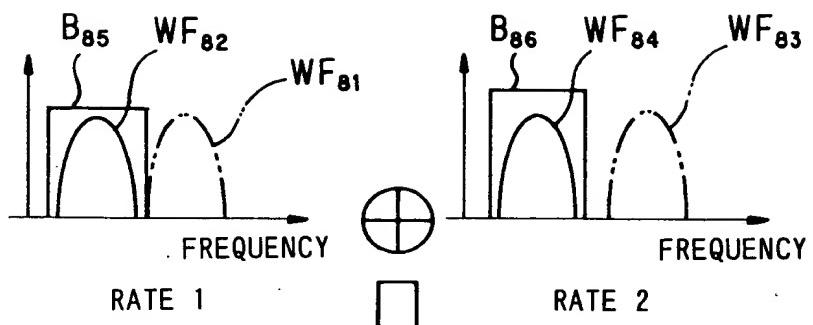

RATE 1

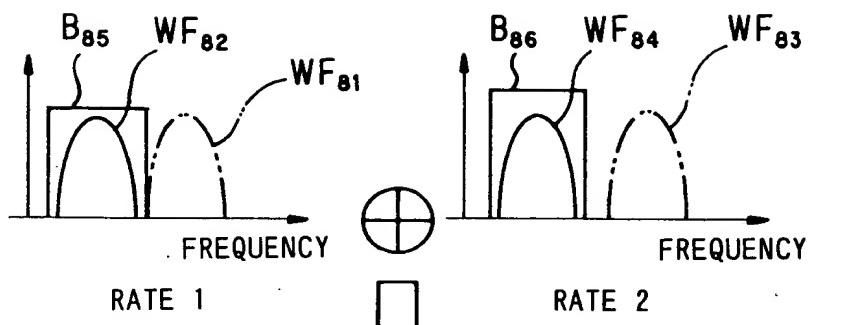

RATE 2

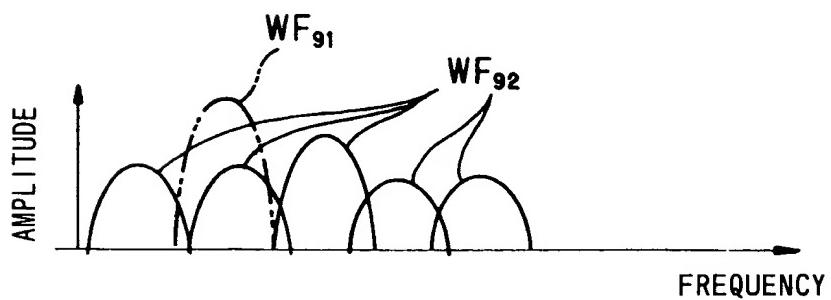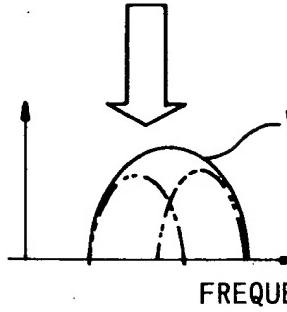

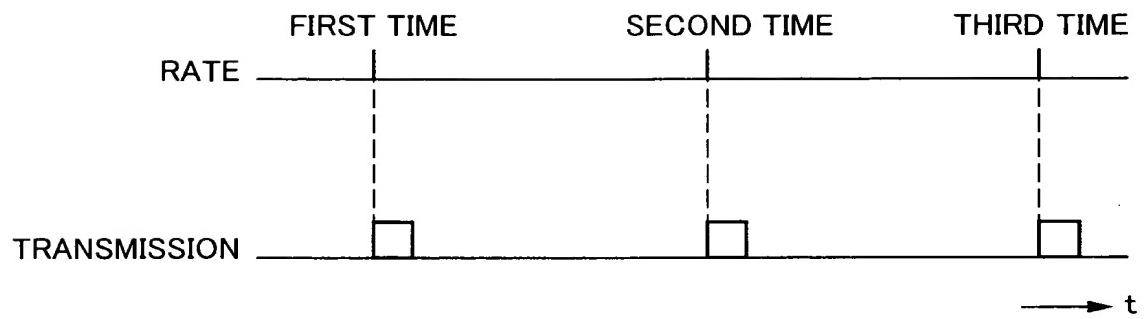


FIG. 11

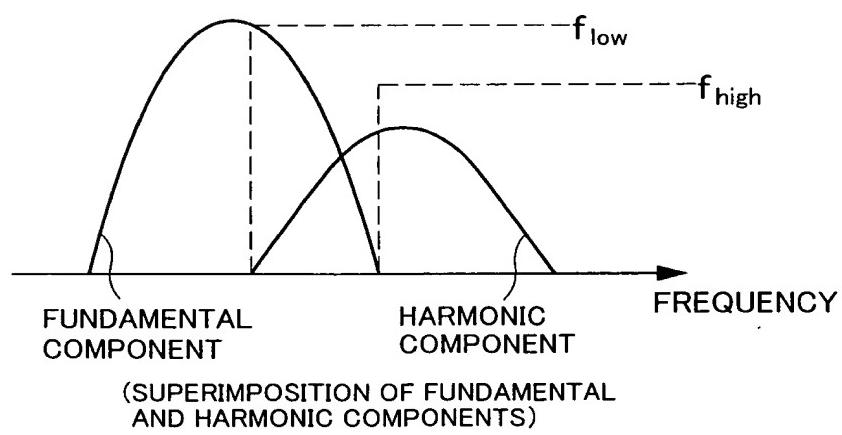


FIG. 12

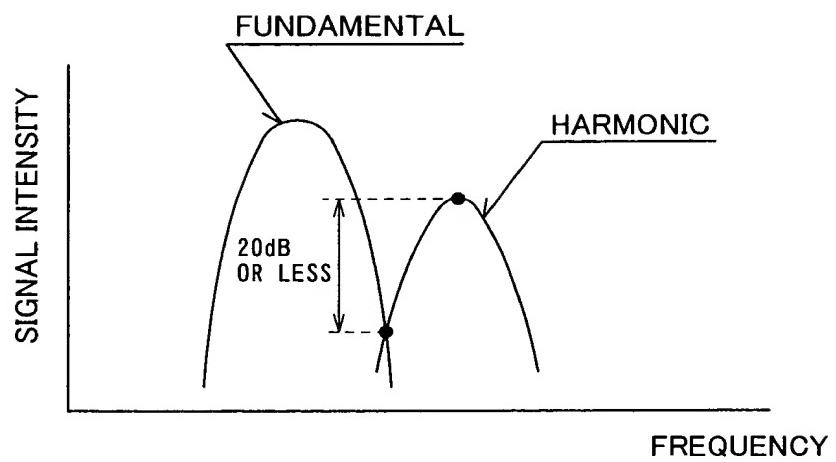


FIG. 13

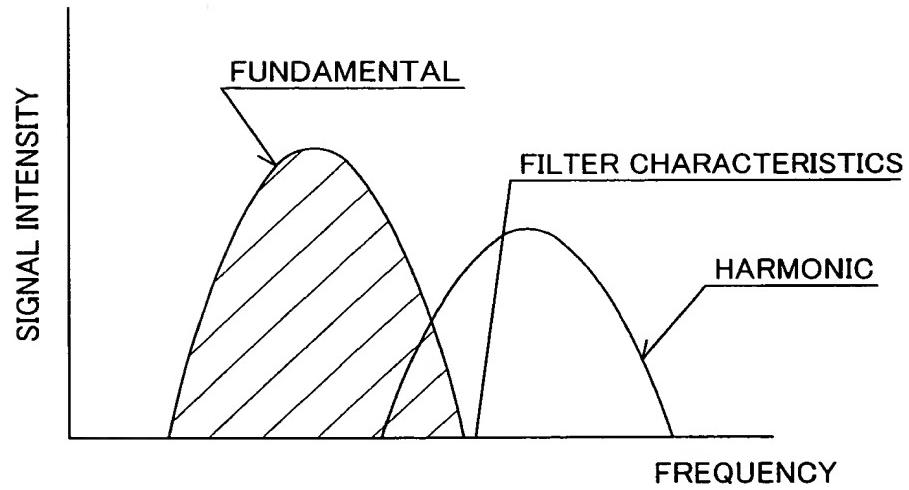


FIG. 14

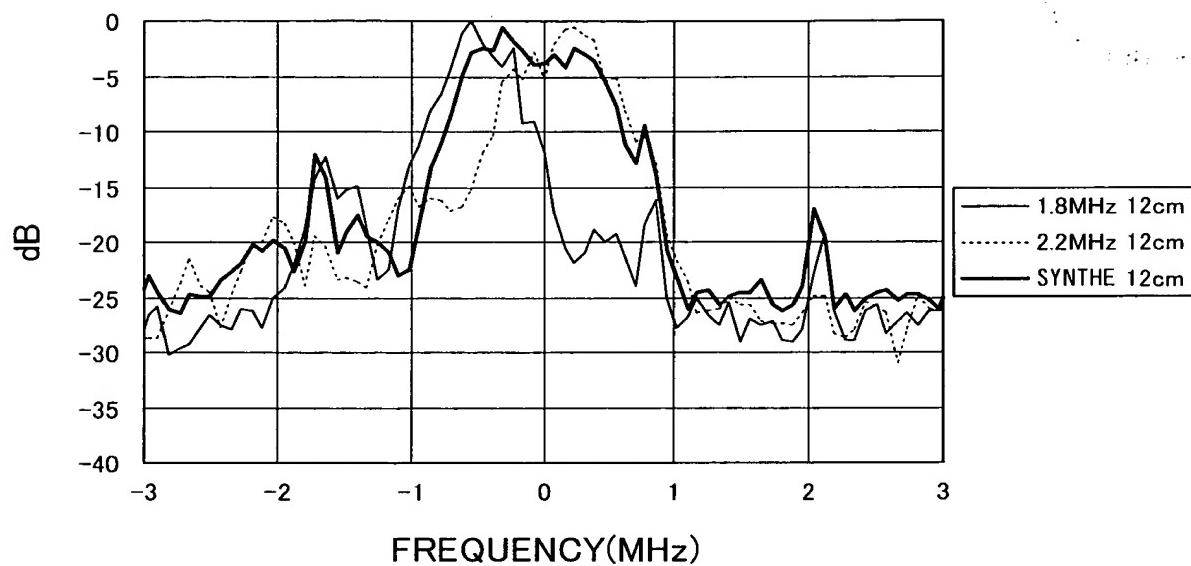


FIG. 15

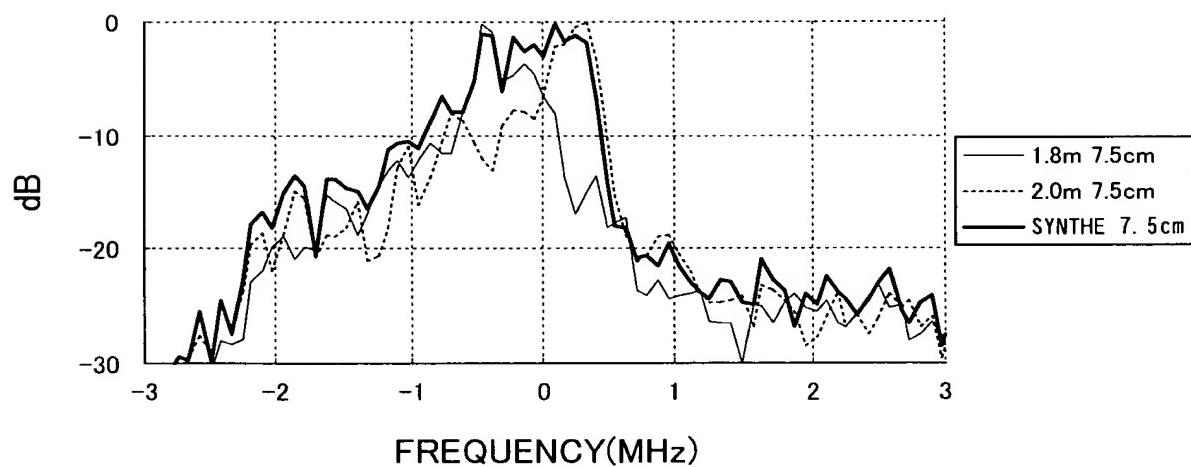


FIG. 16